

A New Digital Stethoscope with Environmental Noise Cancellation

F. BELLONI[†], D. DELLA GIUSTINA[†], M. RIVA[†], M. MALCANGI[#]

[†]Dipartimento di Fisica
Università degli Studi di Milano
Via Celoria 16, 20133 Milano
ITALY

[#]Dipartimento di Informatica e Comunicazione
Università degli Studi di Milano
Via Comelico 39, 20135 Milano
ITALY

federico.belloni@unimi.it, davide.dellagiustina@unimi.it, riva@unimi.it

<http://elettronica.fisica.unimi.it>

malcangi@dico.unimi.it <http://dsprts.dico.unimi.it> <http://www.lim.dico.unimi.it>

Abstract: - A medical instrument for acquisition and analysis of phono-cardiac signals is described in the paper. The proposed system is based on an electronic stethoscope with enhanced performances in environmental noise reduction, achieved by means of two microphones whose signals are combined by an adaptive algorithm. A software tool able to reproduce, visualize and analyze cardiac sounds completes the system. The recorded data and the results of the analysis are stored in a database to build up clinical history of patients and to allow further consultations. A demonstrator of the tool has been realized. Experimental results show significant improvements in noise reduction, when the filtering algorithm is applied. These features make the instrument suited: i) to be employed in very noisy environment, such as ambulance, ii) to help physicians with acoustic diseases, increasing the sound level and showing the phonocardiogram, and iii) to retrieve basic information on the cardiac activity.

Key-Words: - Adaptive filters, System identification, Biomedical signal analysis, Electronic stethoscope, Analysis cardiac sounds.

1 Introduction

In the last century, cardiovascular illnesses are the first death cause in developed countries [1]. For this reason, many efforts have been made in order to develop sophisticated techniques for the early diagnoses of cardiac disorders. The massive diffusion of such techniques has led physicians to a progressive relinquishment of the traditional stethoscope, with a series of major consequences:

- over-crowding of clinics and long waits for examinations;
- increasing in the National Health Service costs;
- not always justified recourse to time-consuming and expensive diagnostic procedure.

This scenario was also supported by some well known disadvantages of the traditional acoustic stethoscope:

- its performances are strictly linked to the audio capability of the user;
- high levels of environmental noise invalidate auscultations;
- analytic comparisons among delayed auscultations are impossible.

Modern electronic stethoscopes [2-6], already available on the market, take advantage of modern technologies to reduce these disadvantages. They allow to adjust the volume of auscultations and to store them on a non volatile

memory (f.i. on a PC). Also, top level devices are mechanically designed to reject most of the environmental noise, even though its electronic cancellation is not usually implemented. Commercial software tools [7,8] for the record, display and replay of acquired sounds are available too.

This paper presents a comprehensive platform [9] which includes both hardware and software and allows to acquire, to organize and to analyze cardiac signals. Fig.1 shows a block scheme of the whole system. The core of the proposed solution is a new digital stethoscope, performing an environmental noise reduction via a distortionless electronic filter. The digital stethoscope is composed of:

- a low noise signal detection system - Acquisition Board (AB) - that acquires the low level heart sound by means of two high sensitive microphones, and adapt it for the analog to digital conversion;
- a processing unit - Processing Board (PB) - which combines the two signals and reduces the noise using a digital adaptive algorithm, described in the next Section. It also contains hardware resources to display and play in real-time the filtered heart sound.

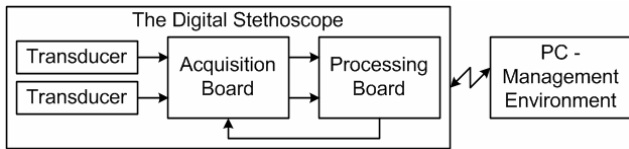


Fig.1. Block scheme of the system.

The AB is placed close to the stethoscope head, while processing section is included in a portable device. In the PB, data are written to a Secure Digital (SD) card and therefore they can be easily copied to a PC, where a software framework stores auscultations into a relational database and allows further consultations.

The paper is organized as follow: Section 2 describes the noise reduction algorithm and the hardware, explaining the limits of traditional approaches. It also introduces the software platform for management and analysis of auscultations. Experimental results are reported in the Section 3 and confirm the effectiveness of the proposed solution.

2 Methods

2.1 Noise Reduction Technique.

One of the most distinctive aspects of the proposed system is its ability to reduce background noise. Several approaches have been proposed in the literature and different solutions were riddled. Some considerations show that many traditional techniques cannot be applied.

The frequency range of the cardiac signal is limited below 1 kHz [10], as shown in Fig.2.

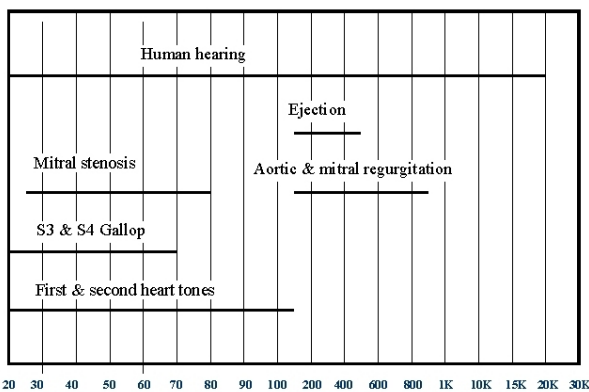


Fig.2. Frequency range of the main cardiac sounds.

The frequency band of the background noise always overlaps this range. To enhance the heart beat x_h with respect to the noise x_n , traditional stethoscopes employ their heads that act as a band-pass filter h_b on the frequency range of interest. Denoting the convolution product by \times , the collected sound is $y = x_h \times h_b + x_n \times h_b$, where the first term of the sum is the actual sound, while the second one is the noise. This process is depicted in Fig.3.

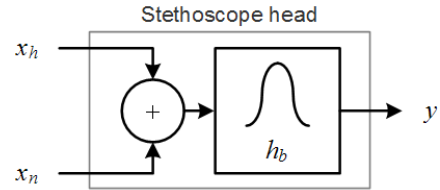


Fig.3. Noise filtering scheme of a traditional stethoscope.

The sound is usable for diagnostic purposes only if the noise is small enough with respect to the heart sound ($\|x_n \times h_b\| \ll \|x_h \times h_b\|$). If this condition is not satisfied, filtering is required. It is worth underlying that physicians are trained to diagnose sounds from traditional stethoscopes so, any further modification of the frequency spectrum, besides those introduced by h_b , can lead to a wrong diagnosis.

The most naive approach to achieve noise reduction should employ a further low-pass electronic filter h_{lp} on the sound $(x_h + x_n) \times h_b$ (Fig.4).

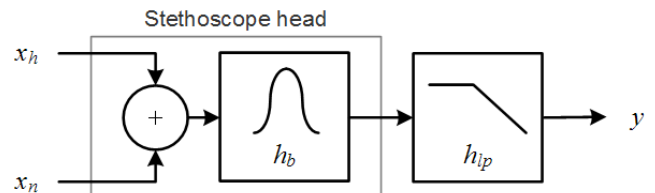


Fig.4. Noise filtering scheme of the elementary solution.

This solution would work if most part of the energy of the background noise was associated to high frequencies. Optimum filtering techniques have been considered too (Fig.5).

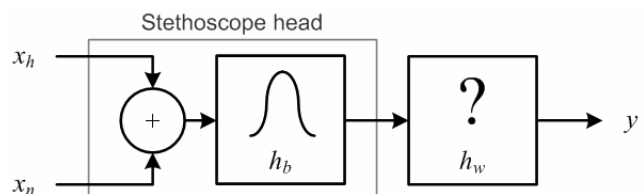


Fig.5. Generic optimum noise filtering scheme.

These algorithms move the noise reduction problem to a dynamic identification problem. Among these latter methods, standard Wiener filtering technique [11] based on a single-channel acquisition is not applicable here, because the noise reduction is strictly linked with a signal distortion that makes impossible a traditional diagnosis. In fact, let h_w be the impulse response of the optimum Wiener filter, the output signal is $y = h_w \times (x_h + x_n) \times h_b$ which is different from the expected signal $x_h \times h_b$. In principle, distortions could be reduced using a multiple-channel algorithm [12]. Nevertheless, in both cases (single and multiple channels) noise has to be estimated in the operative conditions (i.e. when the stethoscope head is applied on the patient's body) without detecting the heart beat. Evidently, such a condition cannot be satisfied. So, standard and multi-channel Wiener

filtering methods cannot be successfully applied.

The approach proposed in the paper uses a stethoscope head equipped with two small pipes. While the first pipe is directly connected to the stethoscope head, the latter is put just beside, as shown in Fig.6.

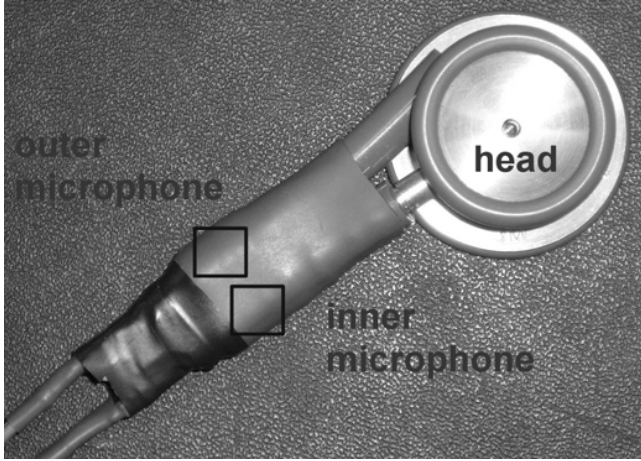


Fig.6. Stethoscope head equipped with the two microphones.

A microphone is placed inside of each pipe. Inner microphone perceives the sound from the inside of the head, i.e., both the heart beat and the noise. Outer microphone detects the noise only, due to the very low level of the cardiac signal (hypothesis experimentally verified). The pipes have the same length and are placed close enough so that the spatial dependencies of the sound waves are negligible in the frequency range of interest.

The filtered signal cannot be easily yielded through a direct subtraction (Fig.7), because the two transducers do not sense the noise in the same way.

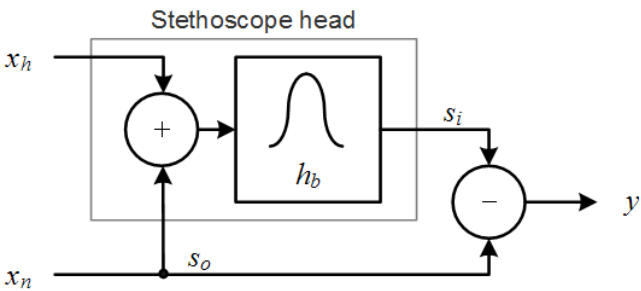


Fig.7. Direct difference method.

Differences between the signals, caused by the stethoscope head and by the interaction with the patient body, must be considered before subtracting (Fig.8). The key point of the described approach is the best estimation of the physical system response h_{wd} .

Its time-variant dynamics depends on:

- type of stethoscope head;
- patient's build and posture;
- position and pressure of the head over the patient's body;
- possible presence of clothes.

So, an adaptive approach must be adopted. In principle, it consists in minimizing the following functional:

$$E(h_{wd}) := \|s_i - s_o \times h_{wd}\|^2 \quad (1)$$

where s_i and s_o are the signals from the inner and outer microphones respectively.

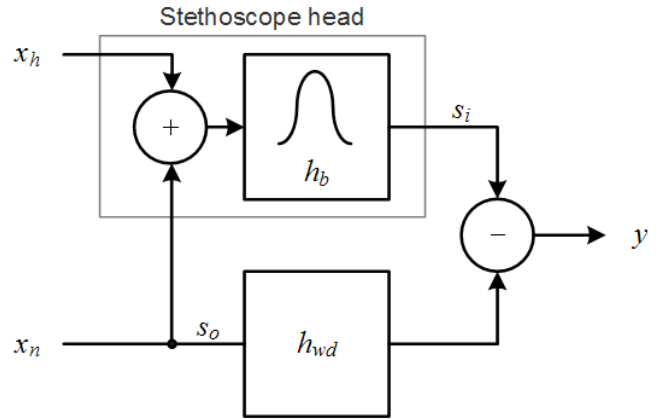


Fig.8. Weighted difference method.

Its numerical implementation can be derived by optimizing the quadratic form (LMS algorithm):

$$E(h_{wd}) = \sum_{k=1}^m \left[s_i(k) - \sum_j s_o(k-j)h_{wd}(j) \right]^2 + \sum_{k=1}^n a(k)h_{wd}^2(k) \quad (2)$$

where n is the number of coefficients of the filter, m is the number of the processed incoming samples and $a(k) > 0$, for all k . The first term in (2) is the numerical translation of (1), while the second term takes into account the energy of the filter itself. Functional (2) admits a unique minimum, that corresponds to the solution of the linear system $h_{wd}A=B$, where

$$A_{ij} := \sum_{k=1}^m s_o(k-j)s_o(k-i) + a(i)\delta(j-i)$$

$$B_{li} = \sum_{k=1}^m s_i(k)s_o(k-i)$$

for $i, j = [1, n]$.

Theoretically, h_{wd} should be updated for each new incoming ADC sample. However, since the dynamic variations of the system are quite slow compared to the sampling frequency, the filter can be calculated only few times per second. This assures a good compliance between the estimated system and the real one, without an excessive computational burden.

Once the target transfer function is correctly estimated, subtraction between the two signals can be carried out without introducing any distortions.

2.2 Hardware Description

A demonstrator of the stethoscope, implementing the noise-reduction technique presented in the previous Section, has been realized according to the general description reported in Fig.1. A detailed description of each part is presented in the following.

2.2.1 Transducers

The first stage of the data acquisition chain consists in a couple of sensors. High sensitive microphones, with flat frequency response in audio range, have to be selected. The devices have to be also small and light not to limit the portability of the instrument. Electret Condenser Microphones (ECM), which completely fulfills the above specifications, have been employed. Moreover, such solution does not require power supply for microphone.

2.2.2 Acquisition Board (AB)

The core of the AB is an analog front-end electronics, which adapts the signals received from the microphones for the AD conversion. According to the block scheme in Fig.9, five main subsystems can be highlighted:

- amplification stages;
- anti-aliasing filter;
- single-ended to differential signal adapter: provides a differential pair to the ADC input;
- feedback network: eliminates the random DC offset voltage of the microphones.

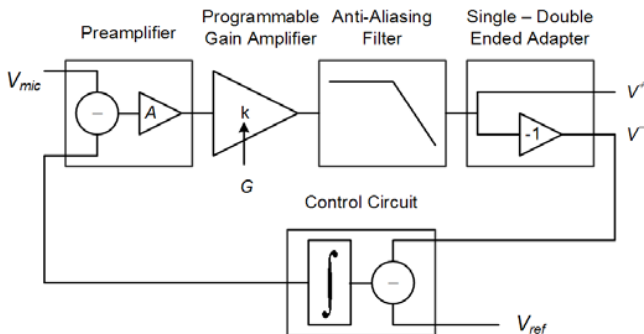


Fig.9. Block scheme of the analog front-end in the AB.

Since the actual signal is derived from the difference between two waveforms of comparable amplitude, a very high signal to quantization noise ratio (SQNR) is required.

In the present implementation, the AB is connected to PB via Ethernet cables to transmit the outputs from the ADC to the PB and the control commands from the PB to ADC.

2.2.3 Processing Board (PB)

The PB, whose block scheme is reported in Fig.10, contains two main digital units: an FPGA and a DSP. The first logic unit coordinates the data transfer from the AB to the PB. Data from ADCs are filtered and stored, so that the DSP can perform the noise reduction algorithm.

The clean heartbeat is then distributed to:

- a DAC, which allows the user to listen to the sound, via common headphones;
- a display, where the sequence is plotted;
- a removable storage media (SD card).

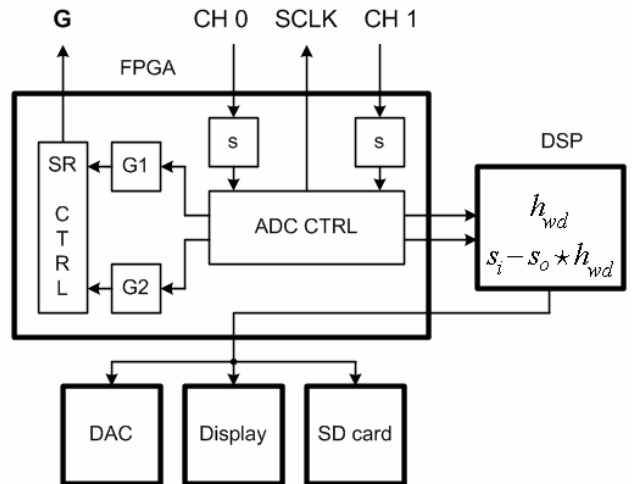


Fig.10. Block scheme of the digital section of the PB.

The DSP has been chosen taking into account that the computational complexity of the algorithm is set by the matrix inversion, $O(n^3)$, and the calculation of A , $O(n^2 m/2)$. The optimum tradeoff between precision and computational time has been obtained updating the filter 4 times per second, i.e., processing chunks of $m = 10000$ samples of the input streams and choosing $n = 400$ filter coefficients.

2.3 Auscultation Management Environment

Auscultation Management Environment (AME) is a software tool constituted by a graphical user interface, shown in Fig.11, and a relational database. It allows the management, the visualization and the playback of the acquired data.

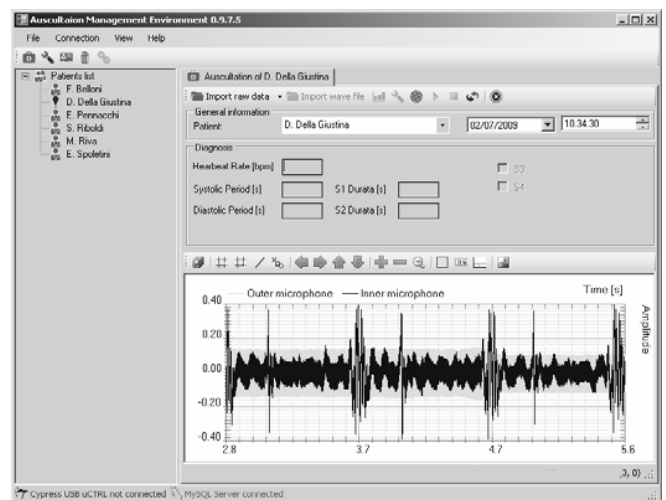


Fig.11. User friendly graphical interface of AME.

A parallel activity of the authors of this paper is focused on designing algorithms to support the automatic diagnosis of cardio-pathologies. The development of these software procedures benefits from high sound quality provided by enhanced stethoscopes. Some functionalities concerning basic cardiac measurements were already integrated in AME. Present research activities, still in progress, are focused on the development of an inferential engine that embeds the physician's ability to execute a diagnosis by hearing, as already discussed in [13] for respiratory sounds. This inferential engine requires features extracted from the cardiac sound by specific functions. Among them, the cardiac cycle isolation (end-pointing) is the most important and challenging. Most of efforts are now focused to setup such capability.

3 Experimental Results

Table 1 and 2 list the main electronic devices employed in the prototypes of the AB and the PB. The demonstrator was tested in various conditions and with different types of noise, to verify the robustness of the filtering algorithm. Besides the typical environmental background noise, such as voices chatting, car motors, horns, fire and ambulance sirens, etc., synthetic noises were considered too. In each situation, a significant noise reduction ratio (NRR) is reached. NRR is defined as the ratio of the power of the signal before and after filtering. Some results are listed in Table 3, where NRR is computed where the heart beat is not present.

Table 1. Main electrical devices in the AB.

Transducers	Knowles Acoustic, EK-3024
Op-Amp	TI, OPA2227
PGA	TI, THS7002
Digital Isolators	Analog Devices, ADuM240x
Low Drop Voltage Regulators	TI, uA78m05,uA79m05
Low Drop Voltage Reference	TI, REF3140
ADC	TI, ADS1252

Table 2. Main electrical devices in the PB.

FPGA	Xilinx, Spartan 3 XC3S200
DSP	TI, TMS320C6726B
Display	OSRAM, OS128064PK16MYO
DAC	TI, PCM1774
DSP Flash Memory	Spansion, S29AL004D
FPGA PROM	Xilinx, XCF02S
Switching Voltage Regulators	TI, TPS61202, TPS62410, TPS65130, TPS61081
Low Drop Voltage Regulators	TI, TPS72301, LP2985
Battery	Ultralife, UBBL07

Table 3. Application of the filtering algorithm: some results.

Environment	NRR dB
Quite office: doors and windows closed; no voices	-12.95
Noisy office: doors and windows open; background voices	- 14.04
Noisy office and synthetic chirp [100 Hz – 2 kHz]	-15.50
Noisy office and low frequency noise	-13.50
Noisy office and high frequency noise	- 16.11
Noisy office and white noise	-14.48

Fig.12 shows the sounds acquired by the inner and the outer microphones when the auscultation is performed with a high frequency synthetic signal superimposed to the typical environmental noise. In such a condition, the acquired cardiac sound is unintelligible. Fig.13 shows the filtered signal after noise cancellation.

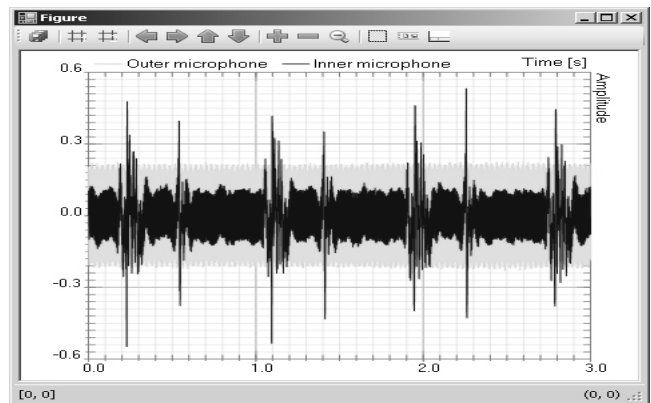


Fig. 12. Comparison between signals from inner and outer microphones.

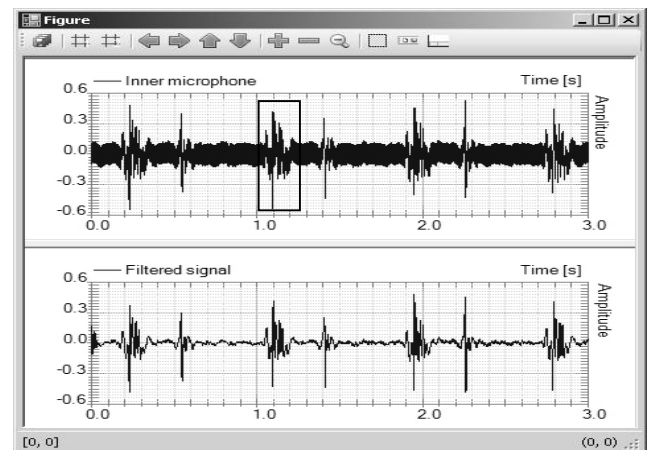


Fig.13. Comparison between inner microphone and filtered signals.

Fig.14 shows a detail of Fig.13. This technique reconstructs the sharp beat peaks while cleaning the superimposed noise at nearly the same frequency.

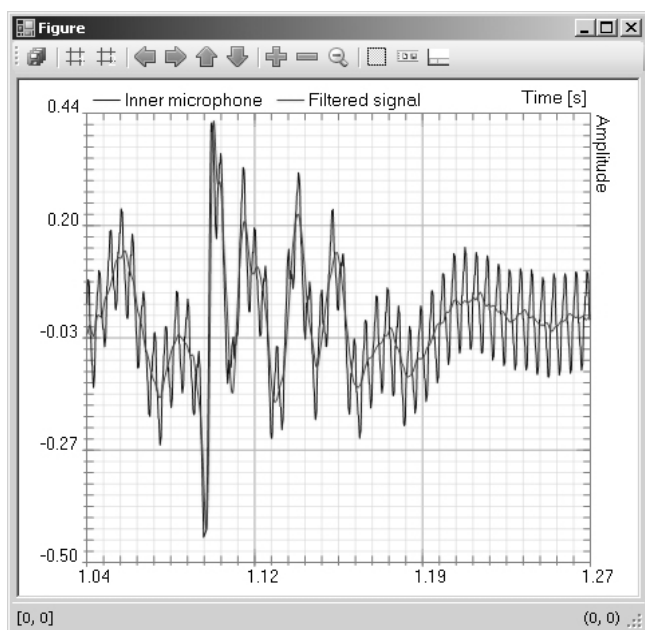


Fig.14. Detail of Fig.13.

4 Conclusions

A new medical equipment for heart sound detection and analysis has been presented. The tool is based upon an electronic stethoscope specifically designed to improve the quality of the auscultation. Noise reduction is achieved acquiring signals from two microphones and applying a weighted difference adaptive algorithm, so that signal is not distort. The electronic hardware is enriched by a software platform to manage auscultations and to provide an assisted diagnosis. Experimental results confirm the accuracy both of the sound detection and of the noise reduction.

References:

- [1]World Health Organization. "Global health indicators - Part 2." Internet: http://www.who.int/whosis/whostat/EN_WHS08_Table1_Mort.pdf, 2008 [Jun. 30, 2009].
- [2]3M™ Littmann®, "Electronic Stethoscope Model 3200", Internet: http://solutions.3m.com/wps/portal/3M/en_US/Littmann/stethoscope/electronic-auscultation/model-3000-series/ [Mar. 11, 2010]
- [3]3M™ Littmann®, "Electronic Stethoscope Model 4100WS with Ambient Noise Reduction", Internet: http://solutions.3m.com/wps/portal/3M/en_US/Littmann/stethoscope/products/product-catalog-us/?PC_7_RJH9U5230GE3E02LECIE20KFI1_nid=QXZZ4ZRZKKbeD77LGQCVJWgl [Mar. 11, 2010]
- [4]Thinklab, "ds32a Digital Electronic Stethoscope" Internet: <http://www.thinklabsmedical.com/> [Mar. 11, 2010]
- [5]Welch Allyn, "Electronic Stethoscope", Internet: http://www.welchallyn.com/apps/products/product_cate gory.jsp?catcode=STS&subcatcode=STS-E [Mar. 11, 2010]
- [6]Texas Instruments, "Digital Stethoscope Solution", Internet: <http://focus.ti.com/docs/solution/folders/print/478.html> [Mar. 11, 2010]
- [7]BioSigenetics Corporation, "Phonocardiograph Monitor Software", Internet: <http://www.bsigenetics.com/> [Mar. 11, 2010]
- [8]Zargis Medical, "Zargis Cardioscan", Internet: <http://www.zargis.com/index-2.php> [Mar. 11, 2010]
- [9]F. Belloni, L. Bertossi, D. Della Giustina, S. Riboldi, M. Riva and E. Spoletini. "Towards a Computer-Aided Diagnosis by means of Phonocardiogram Signals." in *Proc. IEEE-ISIE, 2007*, pp. 2770–2775.
- [10]M.E. Tavel. *Clinical Phonocardiography & External Pulse Recording*. Chicago: Year Book Medical Publishers Inc., third edition, 1978.
- [11]A. V. Oppenheim and R. W. Schaffer. *Discrete-Time Signal Processing*. Englewood Cliffs, NJ: Prentice Hall, second edition, 1989.
- [12]J. Chen, J. Benesty, and Y.A. Huang. "A Minimum Distortion Noise Reduction Algorithm With Multiple Microphones." *IEEE Transaction on Audio, Speech and Language Processing*, vol. 16, no. 3, pp. 481-493, Mar. 2008.
- [13]D. Catania, M. Malcangi and M. Rossi, "Improving the Automatic Identification of Crackling Respiratory Sound Using Fuzzy Logic", *International Journal of Computational Intelligence*, vol. 2, no. 1, Jan 2004.